

InGaAs Ultra-Low Noise Balanced Detector

400M



- **Product Description**

The UBD series ultra-low noise balanced detector module are upgraded products based on the previous MBD series. Compared to the original MBD series, the background noise is significantly reduced under the same conditions. With the same bandwidth and gain, the background noise of the UBD series is approximately one-third of that of the MBD series modules,

resulting in higher sensitivity and better signal-to-noise ratio.

- **Product features**

Ultra-low noise、High Gain、High bandwidth、Compact structure、Built-in

low-noise isolation power supply

- **Part Number**

MP-UBD-M-I-400-F/S-D/A

- **Application area**


Distributed fiber optic sensing、Laser wind radar、Optical coherence

tomography、Spectral measurement、Pulsed light detection

- **Core parameters**

Wavelength	Bandwidth	Responsivity
800-1700nm	400MHz	0.95A/W

● Dimension Drawing

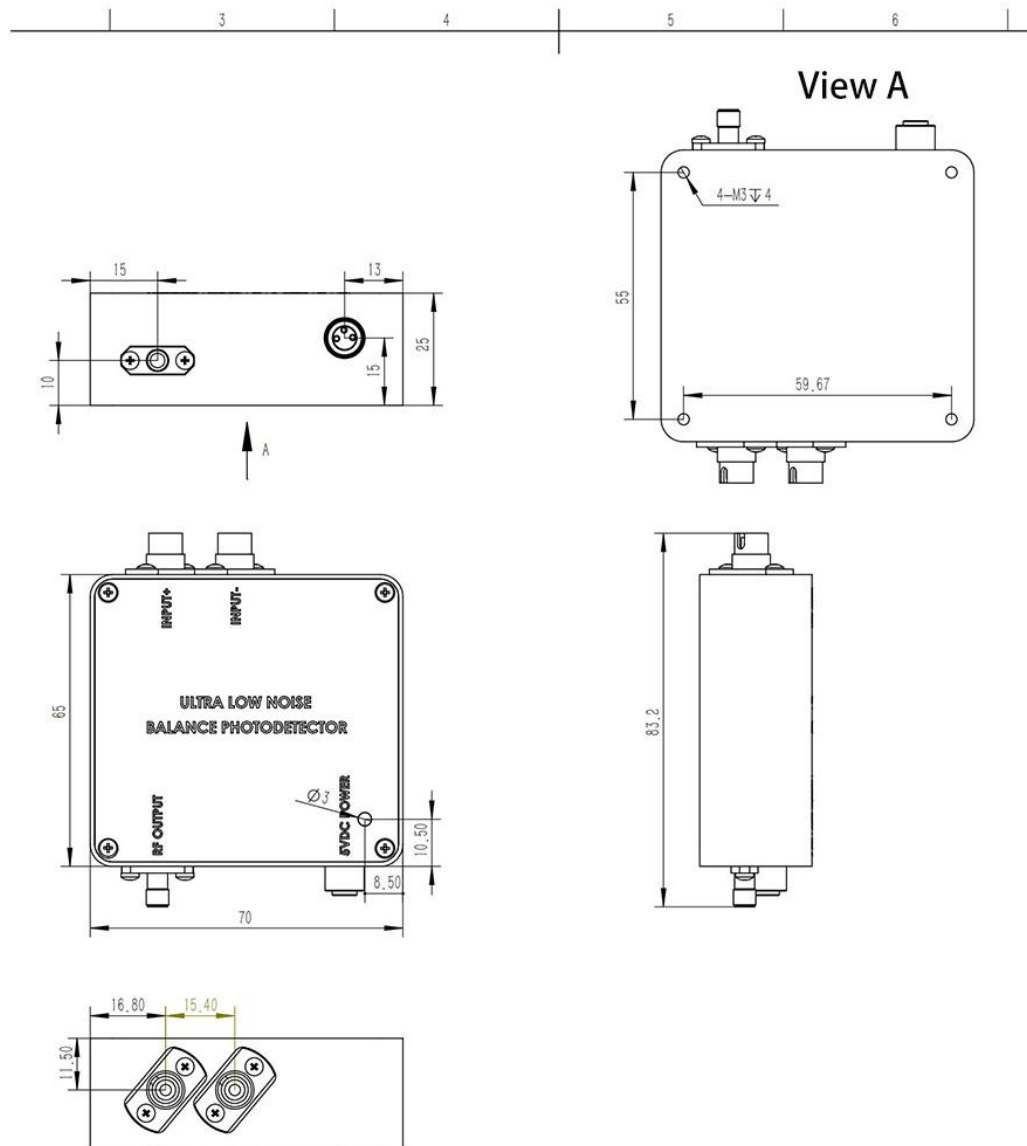

● General Parameters


Parameter

Detect or type	InGaAs											
Wavele ngth	800~1700											nm
Bandw idth	100 M	200 M	300 M	400 M	500 M	800 M	1G	1.2 G	1.5 G	2G	2.5 G	Hz
Detect or respon sivity	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	0.9 5	A/W@ 1550n m
Transi mpeda nce gain	30K	30K	30K	20K	10K	30K	30K	30K	30K	30K	30K	V/W


Maximum input optical power	140	140	140	210	420	140	140	140	140	140	140	μW
NEP	2.5	2.5	2.5	2.9	3.1	3.1	3.1	3.1	3.1	3.1	3.1	pW/S qrt(Hz)
Common mode rejection ratio	>30	>30	>30	>30	>30	>30	>30	>30	>30	>30	>30	dB
Output impedance	50	50	50	50	50	50	50	50	50	50	50	Ω

Output coupling mode	DC/AC	DC/AC	DC/AC	DC/AC	DC	AC	AC	AC	AC	AC	AC	
Supply voltage	5	5	5	5	5	12	12	12	12	12	12	V
Supply current	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	0.5(max)	A
Optical input	FC/APC (Free space optional)											
RF output	SMA											
Dimensions	80*90*25											mm

Test result

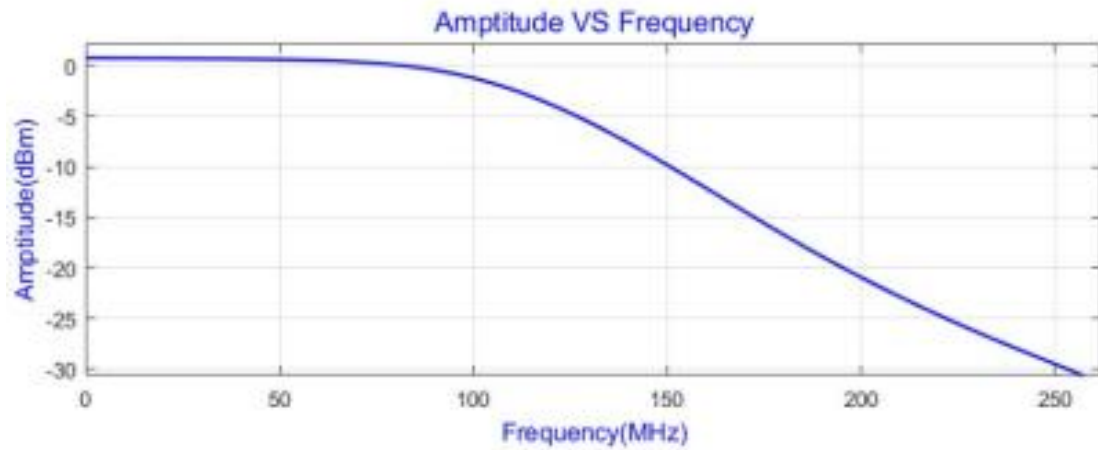

300 MHz bandwidth response curve

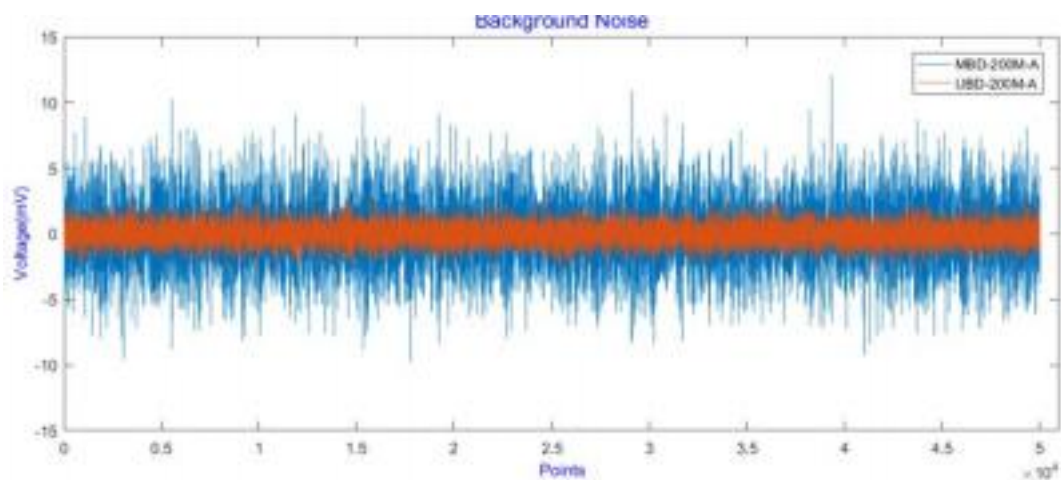

Comparison of the baseline noise between ultra-low noise balanced detectors
and conventional balanced detectors